

Vertical Bone Augmentation with Simultaneous Dental Implantation Using Crestal Biomaterial Rings: A Rabbit Animal Study

Florian G. Draenert, MD, DDS, PhD;* Peer W. Kämmerer, MD, DDS;† Victor Palarie, MD, DDS;‡ Wilfried Wagner, MD, DDS, PhD‡

ABSTRACT

Background: Ceramic biomaterial blocks like hydroxyl apatite are too brittle for simple simultaneous vertical augmentation and dental implant placement. Biological scaffolds of xenogenic or allogenic origin are known to be advantageous.

Purpose: The aim of this study was the proof of principle for combined vertical bone augmentation and dental implantation with marginal cuffs made of biological scaffolds with interconnecting porous system and titanium dental implants.

Materials and Methods: Cylindrical porcine biomaterial rings (processed, mineralized bone matrix) were placed in combination with titanium dental implants in the tibia model using six chinchilla bastard rabbits ($n = 12$ samples). Histological examination included undecalcified histological examination with toluidine blue staining and fluorescence microscopy. Animals were sacrificed after 30 days.

Results: The results showed bony healing in the scaffolds with immature bone tissue ingrowth following the trabecular structure, showing lamellar cancellous bone healing. Fluorescence microscope showed analogous results.

Conclusion: The biological scaffold proved a biocompatibility in a xenogenic setting. The vertical bone augmentation with simultaneous implantation was successful and proved the feasibility of the concept.

KEY WORDS: biomaterials, rabbit, vertical bone augmentation

INTRODUCTION

Successful functional and esthetic placement of dental implants requires a sufficient bony bed in the jaws. The loss of teeth can lead to various defects in the bone resulting from different pathological mechanisms.¹ Periodontal inflammation, pressure of removable prosthetics, and physiological resorption in the edentulous jaws lead to various, mostly combined, defects, including horizontal and vertical bony deficiency. Whereas horizontal defects allow standard guided bone regeneration (GBR) techniques and similar approaches, it is necessary to provide mechanical stability in vertical defects.^{2–6}

*Associate professor, Clinic for Oral & Maxillofacial Surgery, University of Mainz, Mainz, Germany; †assistant professor, Clinic for Oral & Maxillofacial Surgery, State Medical and Pharmaceutical University “Nicolae Testemitanu,” Chisinau, Moldova; ‡chairman, Clinic for Oral & Maxillofacial Surgery, University of Mainz, Mainz, Germany

Reprint requests: Dr. Florian G. Draenert, Augustusplatz 2, 55131 Mainz, Germany; e-mail: draenert@floriandraenert.com

© 2011 Wiley Periodicals, Inc.

DOI 10.1111/j.1708-8208.2011.00401.x

Vertical bone augmentation is still a challenging problem in dental implantology.^{1,3–5,7} The most common techniques for these surgeries are bone block grafts, distraction osteogenesis or particulate biomaterials, and bone in combination with either sandwich osteoplastic or membrane techniques (GBR).^{2,6,8–17} Other options are cylindrical autologous bone grafts as presented previously.^{18,19} The use of bone cylinders and rings derived from the well-known technique of trephine drill harvesting for bone grafts.^{20,21} Using these graft designs allows to prepare appropriate implant sites for better fit compared with the hand crafted block grafts.^{18–23}

The use of these graft types in dental implantology can be diverted in the trias of bone ring cuffs around implant necks, assisted press-fit cylinders with osteosynthesis screw fixation, and those with press-fit not requiring a screw as discussed earlier.¹⁸ The later ones demand a second procedure for the placement of a dental implant. The first approach bears several advantages including the on-step procedure. However, the

harvesting of the graft results in donor site morbidity. Using alloplastic, allogenic or xenogenic materials could avoid this second injury for the patient. Additionally, it was histologically shown that autologous cortical bone grafts show only limited osseous healing in rabbits.²⁴ This implies that a cancellous structure with interconnecting pores could be a better option. We referred to previous clinical results with vertical bone augmentation, used a processed cancellous bone material described earlier as cuff ring for simultaneous vertical bone augmentation in the rabbit tibia model, and evaluated bony healing in this type of bone augmentation.^{18,25}

MATERIALS AND METHODS

Experimental Setup

The animal study of a biphasic implant consisting of a cancellous bone-derived material ring and a commercial dental implant was done in six chinchilla bastard rabbits using the tibia model on both sides ($n = 12$ samples). Samples were taken after 30 days representing the final acute bone healing in rabbits.

Preparation of the Biphasic Implant Device

Steam-resistant mineralized bone matrix (SMBM) was obtained by the preparation process described earlier.²⁵ This technique involves mechanical cleaning, defatting, and steam sterilization without enzymatic fermentation. We used cancellous bone from the porcine pelvic bone (Mainz slaughter house, Germany). The bone rings were harvested using diamond hollow drills (diamond trephine control system, Hager & Meisinger Inc., Neuss, Germany). Bone cylinders measuring 7.5 mm (diameter) x 2.0 mm (height) were obtained by drilling the bone blocks at an angle of 90° with a diamond drill size of 8.0 mm (outer diameter) and then cutting to the correct length with a scalpel. Alfa Gate Bioactive titanium implants with calcium phosphate coating were obtained from the company as free samples (Alfa Gate Dental Implants, Kfar Qari, Israel). The biphasic implant consisting of both parts was assembled under sterile conditions under the laminar flow bench (see Figure 1). Samples were stored at -30°C before surgery.

In Vivo Experiments

The animal experiments were approved by the government of Moldova and performed in compliance with the



Figure 1 Biphasic implant consisting of a porcine steam-resistant mineralized bone matrix ring and an Alfa Gate 3.75/8 mm SCI implant (VHX-600 digital three-dimensional microscope, Keyence Inc., Osaka, Japan).

guidelines for animal experimentation in the animal experimentation institute of the University of Moldova (Chisinau, Moldova). Female ex-breeder chinchilla bastard rabbits were chosen for all experiments as their growth plates were closed, which ensured normal bone healing. The animals were held in a combined indoor and outdoor paddock containing up to four rabbits each; the rabbits had unrestricted mobility. The number of rabbits was chosen according to the standards in medical device research for representative descriptive histology. Anesthesia included ketamine 100 mg/xylazine 20 mg/5 kg adapted to the individual weight of the animal. The biphasic implants were placed in both medial tibia bones of the six animals via an anterior transdermal approach ($n = 12$ samples) following the drill protocol of the manufacturer after planar drilling of the bone surface with a planar drill (Ring Control Professional System, Hager & Meisinger Inc., Neuss, Germany). Wound closure included running sutures using Vicryl 3-0 (Ethicon, Inc., Somerville, NJ, USA). Animals received up to 30 mg phenylbutazone after the operation. The rabbits were sacrificed by an overdose of ketamine 200 mg decapitation. Samples were harvested and fixated with 4% paraformaldehyde.

Histological Examination

Samples were cut in appropriate bony pieces after immersion fixation for 4 weeks as described earlier. Histological preparation was described elsewhere.^{26,27} Dehydration

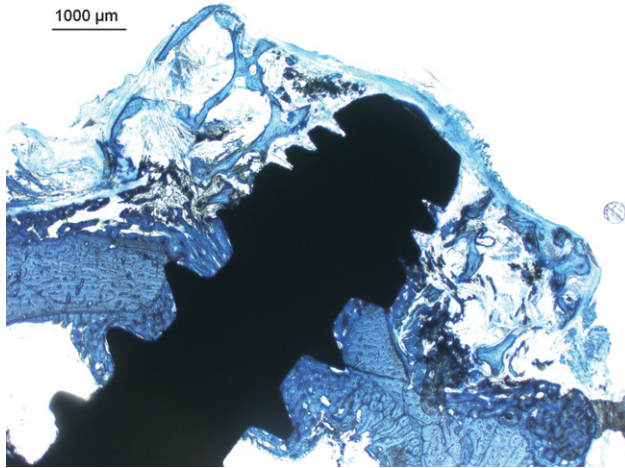


Figure 2 Histological example with toluidine blue staining (50×) showing early lamellar bone healing and marginal bone mineralization.

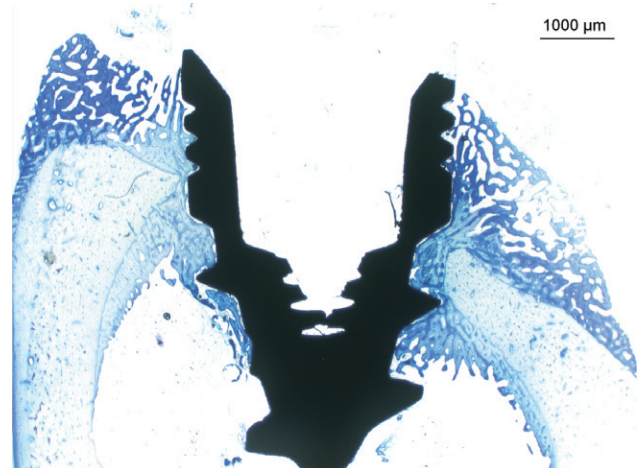


Figure 3 Histological example with toluidine blue staining (50×) showing advanced immature bony healing and mineralization of marginal triangle area.

with increasing percentages of alcohol (70–100%) was followed by Technovit® embedding (Heraeus Kulzer GmbH & Co., Wehrheim, Germany), toluidine blue staining, and diamond grinding of microscopic samples down to a thickness of 20 μm. Light and fluorescence microscopic examination was performed under a Leica DM8000 M microscope (Leica Microsystems GmbH, Wetzlar, Germany). Pigs are regularly treated with tetracycline resulting in fluorescence of the porcine mineralized bone matrix (SMBM) used in this study. This effect was applied to show newly formed bone (no fluorescence) within the fluorescence-marked biomaterial more clearly. Data were analyzed as means and standard deviations. ‘Prism’ version 5.0d (GraphPad Software Inc., La Jolla, CA, USA) was used for the analysis.

RESULTS

Light Microscopic Examination

Samples showed a good osseointegration of the titanium implant in the local bone in all samples (see Figures 2 and 3). Examination of the biomaterial rings showed bone ingrowth with most mature mineralization in the marginal bone area forming a mineralization triangle from the local bone surface toward the supracrestal implant surface. The structure of the scaffold material was either completely replaced by newly formed cancellous bone or in the process of ingrowth. Most mature bone with advanced mineralization was observed in the marginal bone triangle between supracrestal rough implant body and the horizontal, marginal, crestal bone.

Fluorescence Microscopic Examination

Corresponding fluorescence examination showed newly mineralized bone tissue in the described triangular area as well as in the implant interface in all samples (see Figure 4). The newly mineralized, marginal, vertical bone growth was measured (see Figure 5). The height of

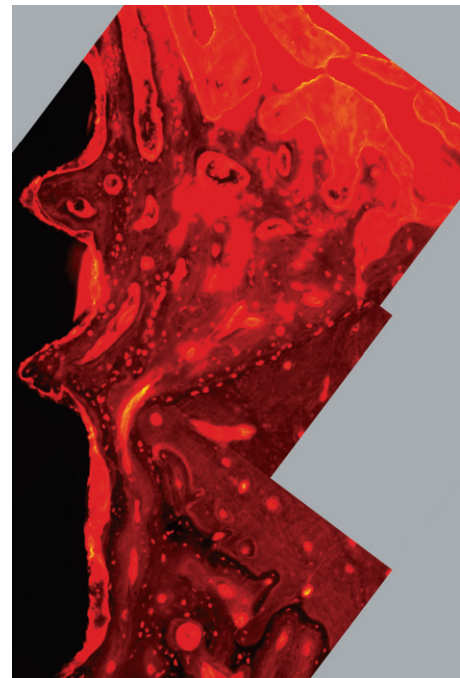


Figure 4 Fluorescence microscopy emphasizes the newly formed marginal bone due to remains of the matrix fluorescence (200×, assembled from multiple images following digital mosaic technique).

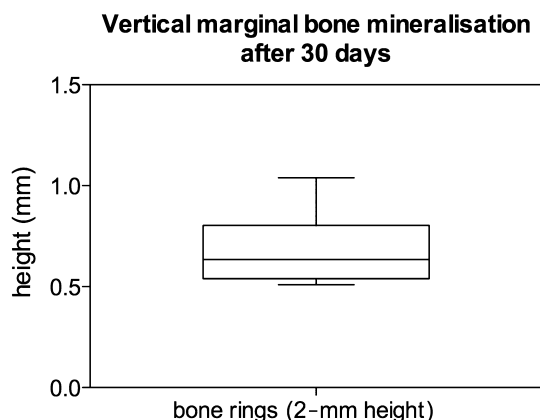


Figure 5 Vertical, marginal mineralized bone growth height with mean and standard deviation.

the newly formed mineralized bone was between 0.51 and 1.04 mm (mean 0.68 mm), covering the rough surface of the implant completely. [Correction added to online publication 12 December 2011]

DISCUSSION

Samples were taken after 30 days representing the end of acute bony healing in rabbits.^{25,28,29} The rabbit tibia is an accepted animal model for biomaterial research and technically favorable.^{30–32} Therefore, it was the preferred choice. The Alfa Gate dental implants are advantageous for bony healing due to their calcium phosphate coating.³³ The biocompatibility of the SMBM material was proved in an earlier study and was reproducible in this experiment.²⁵ Bony ingrowth and mineralization was fast following the cancellous SMBM scaffold structure. The use of porcine material also proved biocompatibility of the SMBM processing in xenogenic bone biomaterials. This has some impact on actual product developments such as the equine bone block from Geistlich Inc. (Wolhusen, CH, Switzerland) and supports the idea of xenogenic biomaterials.³⁴ This pilot study provides valid descriptive data. We also analyzed the vertical mineralized marginal bone growth with mean and standard deviation. However, due to the limited size and structure volatility, these data must be considered as preliminary. Metric data with high statistic power demand more animals and a cancellous bone model like the patellar groove to avoid influence of surrounding muscle movements as given in the tibia model.³⁵

A previous study in rabbits showed a limited healing of cylindrical autologous bone grafts fixed with osteosynthesis screws after 3 months, indicating an uncertain fate for the cortical bone rings described for vertical

augmentation in several publications clinically as mentioned earlier.²⁴ This study reported fibrous healing in the interface in 50% of the cases and complete fibrous resorption of the bone transplant in another 50% of the cases.²⁴ The aim of our current animal study was to evaluate the option of cancellous bone material processed from xenogenic bone. The histological results indicate a successful osseous healing in all cases with a complete immature bone tissue ingrowth. Beginning calcification can be observed in the marginal bone triangle as typical location for this process. These results support the current clinical success of vertical bone augmentation with this kind of material in our group (unpublished data) and emphasize the importance of a cancellous structure with interconnecting pores for vertical bone augmentation materials.

Biomaterial blocks offer advantages compared with particulate vertical bone augmentation.^{11,16,36} No stabilizing medical devices such as titanium mesh or metal-enhanced membranes are required. Reduced resorption of block grafts was compared with particulate augmentation with GBR techniques.³⁷ Osteosynthesis screws are a disadvantage of most block augmentations. However, this can be avoided if the dental implant is placed simultaneously or a press-fit is achieved.^{18,19} The need for bone grafts or bone-derived materials containing protein matrix derives from the strong stress within the material block when performing simultaneous implantation. Alloplastic materials such as hydroxylapatite, tricalciumphosphate, and others are too brittle concerning internal stress forces, resulting in fracture of the material block. Using bone-derived biomaterial matrices with mechanical stiffness avoids donor site morbidity resulting from the harvesting of autologous bone blocks.

CONCLUSION

The results of this pilot study show that vertical bone augmentation using a biological scaffold with interconnecting porous system of a cancellous structure combined with simultaneous dental implant placement is successful in the rabbit tibia model. It results in good bony ingrowth of scaffold and osseointegration of the dental implant.

REFERENCES

1. Cawood JI, Stoelinga PJ, Blackburn TK. The evolution of preimplant surgery from preprosthetic surgery. *Int J Oral Maxillofac Surg* 2007; 36:377–385.

2. Buser D, Dula K, Hess D, Hirt HP, Belser UC. Localized ridge augmentation with autografts and barrier membranes. *Periodontol* 2000 1999; 19:151–163.
3. Khoury F, Buchmann R. Surgical therapy of peri-implant disease: a 3-year follow-up study of cases treated with 3 different techniques of bone regeneration. *J Periodontol* 2001; 72:1498–1508.
4. Raghoobar GM, Timmenga NM, Reintsema H, Stegenga B, Vissink A. Maxillary bone grafting for insertion of endosseous implants: results after 12–124 months. *Clin Oral Implants Res* 2001; 12:279–286.
5. Rocchietta I, Fontana F, Simion M. Clinical outcomes of vertical bone augmentation to enable dental implant placement: a systematic review. *J Clin Periodontol* 2008; 35:203–215.
6. Steinhauser E, Obwegeser H. Rebuilding the alveolar ridge with bone and cartilage autografts. *Trans Int Conf Oral Surg* 1967; 1:203–208.
7. Tinti C, Parma-Benfenati S, Polizzi G. Vertical ridge augmentation: what is the limit? *Int J Periodontics Restorative Dent* 1996; 16:220–229.
8. Dahlin C, Linde A, Gottlow J, Nyman S. Healing of bone defects by guided tissue regeneration. *Plast Reconstr Surg* 1988; 81:672–676.
9. Esposito M, Grusovin MG, Kwan S, Worthington HV, Coulthard P. Interventions for replacing missing teeth: bone augmentation techniques for dental implant treatment. *Cochrane Database Syst Rev* 2008; (3):CD003607.
10. Felice P, Marchetti C, Iezzi G, et al. Vertical ridge augmentation of the atrophic posterior mandible with interpositional bloc grafts: bone from the iliac crest vs. bovine anorganic bone. Clinical and histological results up to one year after loading from a randomized-controlled clinical trial. *Clin Oral Implants Res* 2009; 20:1386–1393.
11. Khoury F, Antoun H, Missika P. Bone augmentation in oral implantology. New Malden, UK: Quintessence Publishing Co. Ltd, 2006.
12. Klesper B, Lazar F, Siessegger M, Hidding J, Zoller JE. Vertical distraction osteogenesis of fibula transplants for mandibular reconstruction – a preliminary study. *J Craniomaxillofac Surg* 2002; 30:280–285.
13. McAllister BS, Gaffan TE. Distraction osteogenesis for vertical bone augmentation prior to oral implant reconstruction. *Periodontol* 2000 2003; 33:54–66.
14. Rocuzzo M, Ramieri G, Bunino M, Berrone S. Autogenous bone graft alone or associated with titanium mesh for vertical alveolar ridge augmentation: a controlled clinical trial. *Clin Oral Implants Res* 2007; 18:286–294.
15. Schettler D, Holtermann W. Clinical and experimental results of a sandwich-technique for mandibular alveolar ridge augmentation. *J Maxillofac Surg* 1977; 5:199–202.
16. Tonetti MS, Hammerle CH. Advances in bone augmentation to enable dental implant placement: Consensus Report of the Sixth European Workshop on Periodontology. *J Clin Periodontol* 2008; 35:168–172.
17. Urban IA, Jovanovic SA, Lozada JL. Vertical ridge augmentation using guided bone regeneration (GBR) in three clinical scenarios prior to implant placement: a retrospective study of 35 patients 12 to 72 months after loading. *Int J Oral Maxillofac Implants* 2009; 24:502–510.
18. Draenert FG, Huetzen D, Kämmerer P, Wagner W. Bone augmentation in dental implantology using press-fit bone cylinders and twin-principle diamond hollow drills: a case series. *Clin Implant Dent Relat Res* 2011; 13:238–243.
19. Giesenhausen B. Die einzeitige vertikale augmentation mit ringförmigen knochentransplantaten. *Z Zahnärztl Implantol* 2008; 24:43–46.
20. Sandor GK, Nish IA, Carmichael RP. Comparison of conventional surgery with motorized trephine in bone harvest from the anterior iliac crest. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod* 2003; 95:150–155.
21. Sandor GK, Rittenberg BN, Clokie CM, Caminiti MF. Clinical success in harvesting autogenous bone using a minimally invasive trephine. *J Oral Maxillofac Surg* 2003; 61:164–168.
22. Draenert GF, Ehrenfeld M, Eisenmenger W. [A new technique for transcrestal sinus floor elevation with press-fit bone cylinders (dowel lift): short communication of the first in vitro results]. *Mund Kiefer Gesichtschir* 2007; 11:43–44.
23. Draenert GF, Eisenmenger W. A new technique for the transcrestal sinus floor elevation and alveolar ridge augmentation with press-fit bone cylinders: a technical note. *J Craniomaxillofac Surg* 2007; 35:201–206.
24. Cordioli G, Atiyeh F, Piattelli A, Majzoub Z. Healing of transplanted composite bone grafts-implants: a pilot animal study. *Clin Oral Implants Res* 2003; 14:750–758.
25. Draenert GF, Delius M. The mechanically stable steam sterilization of bone grafts. *Biomaterials* 2007; 28:1531–1538.
26. Donath K, Breuner G. A method for the study of undecalcified bones and teeth with attached soft tissues. The Sage-Schliff (sawing and grinding) technique. *J Oral Pathol* 1982; 11:318–326.
27. Wagner W, Tetsch P, Ackermann KL, Bohmer U, Dahl H. [Animal experimental studies on bone regeneration in standardized defects after the implantation of tricalcium phosphate ceramic]. *Dtsch Zahnärztl Z* 1981; 36:82–85.
28. Nunamaker DM. Experimental models of fracture repair. *Clin Orthop Relat Res* 1998; 456:S56–S65.
29. Stetzer K, Cooper G, Gassner R, Kapucu R, Mundell R, Mooney MP. Effects of fixation type and guided tissue regeneration on maxillary osteotomy healing in rabbits. *J Oral Maxillofac Surg* 2002; 60:427–436. Discussion 436–437.
30. Calvo-Guirado JL, Delgado-Ruiz RA, Ramirez-Fernandez MP, Mate-Sanchez JE, Ortiz-Ruiz A, Marcus A. Histomorphometric and mineral degradation study of Ossceram®: a novel biphasic B-tricalcium phosphate, in critical size defects

- in rabbits. *Clin Oral Implants Res* 2011. DOI: 10.1111/j.1600-0501.2011.02193.x.
31. Joosten U, Joist A, Gosheger G, Liljenqvist U, Brandt B, von Eiff C. Effectiveness of hydroxyapatite-vancomycin bone cement in the treatment of *Staphylococcus aureus* induced chronic osteomyelitis. *Biomaterials* 2005; 26:5251–5258.
32. Liljensten EL, Attaelmanan AG, Larsson C, et al. Hydroxyapatite granule/carrier composites promote new bone formation in cortical defects. *Clin Implant Dent Relat Res* 2000; 2:50–59.
33. Fontana F, Rocchietta I, Addis A, Schupbach P, Zanotti G, Simion M. Effects of a calcium phosphate coating on the osseointegration of endosseous implants in a rabbit model. *Clin Oral Implants Res* 2011; 22:760–766.
34. Simion M, Nevins M, Rocchietta I, et al. Vertical ridge augmentation using an equine block infused with recombinant human platelet-derived growth factor-BB: a histologic study in a canine model. *Int J Periodontics Restorative Dent* 2009; 29:245–255.
35. Draenert GF, Draenert K, Tischer T. Dose-dependent osteoinductive effects of bFGF in rabbits. *Growth Factors* 2009; 27:419–424.
36. Khoury F. Augmentation of the sinus floor with mandibular bone block and simultaneous implantation: a 6-year clinical investigation. *Int J Oral Maxillofac Implants* 1999; 14:557–564.
37. Simion M, Jovanovic SA, Tinti C, Benfenati SP. Long-term evaluation of osseointegrated implants inserted at the time or after vertical ridge augmentation. A retrospective study on 123 implants with 1–5 year follow-up. *Clin Oral Implants Res* 2001; 12:35–45.

Copyright of Clinical Implant Dentistry & Related Research is the property of Wiley-Blackwell and its content may not be copied or emailed to multiple sites or posted to a listserv without the copyright holder's express written permission. However, users may print, download, or email articles for individual use.