

Reduction of biofilm on orthodontic brackets with the use of a polytetrafluoroethylene coating

A. Demling*†, C. Elter**†, T. Heidenblut****, Fr-W. Bach****, A. Hahn***, R. Schwestka-Polly*, M. Stiesch** and W. Heuer**

Departments of *Orthodontics, **Prosthetic Dentistry and Biomedical Materials Science and ***Biostatistics, Hannover Medical School, ****Institute of Materials Science, Leibniz University, Hannover, Germany

†These authors contributed equally to the study.

SUMMARY Treatment with fixed orthodontic appliances can cause enamel demineralization by increased biofilm adhesion. The purpose of the present study was to investigate whether a polytetrafluoroethylene (PTFE) coating reduces biofilm formation on orthodontic brackets.

One PTFE-coated bracket and one uncoated stainless steel bracket were bonded symmetrically on the first or second (four maxillary and nine mandibular) primary molars in 13 adolescent patients (five females and eight males, aged 11.2 ± 2.8 years; four dropouts) for 8 weeks. Quantitative biofilm formation on brackets was analysed with the Rutherford backscattering detection (RBSD) method, a scanning electron microscopy technique. A total of five RBSD micrographs were obtained per bracket with views from the buccal, mesial, distal, cervical, and occlusal aspects. A two-sided paired *t*-test was used to compare data. A *P*-value less than 0.05 was considered significant.

Total biofilm formation was 4.0 ± 3.6 per cent of the surface on the PTFE-coated brackets and 22.2 ± 5.4 per cent on uncoated brackets. Differences between the two groups were statistically significant ($P < 0.05$). Pairwise comparison of biofilm formation with respect to location (buccal, mesial, distal, cervical, and occlusal) revealed a significantly lower biofilm accumulation on PTFE-coated brackets on all surfaces.

The results indicate that PTFE coating of brackets reduces biofilm adhesion to a minimum and might have the potential to reduce iatrogenic side effects, e.g. decalcification during orthodontic treatment with fixed appliances.

Introduction

Treatment with fixed orthodontic appliances allows three-dimensional correction of malocclusions. Compared to treatment with removable appliances, fixed orthodontic therapy affords non-compliance treatment and superior efficacy in terms of treatment time and treatment results (Tang and Wei, 1990).

However, the detrimental effects of fixed therapy can be observed in the short- and long-term. Bracket insertion induces ecological changes of the oral microbiota by affecting its amount, composition, metabolic activity, and pathogenicity, which clinically results in a higher incidence of periodontal disease and incipient carious lesions (Atack *et al.*, 1996; Naranjo *et al.*, 2006; Ahn *et al.*, 2007; van Gastel *et al.*, 2008). In contrast to periodontal and microbial side-effects of fixed orthodontic treatment, which are considered to be largely reversible, signs of previous decalcification resulting in persisting white spot lesions can be observed even long-term after completion of treatment (Øgaard, 1989; Sallum *et al.*, 2004).

These side-effects of fixed orthodontic therapy can be explained by the higher number of plaque-retentive sites and impaired mechanical plaque removal after bracket insertion (Boyd, 1983). In clinical studies, an influence of the bracket material used was also shown to affect intraoral biofilm formation, as well as surface properties of the brackets used (Fournier *et al.*, 1998; Anhoury *et al.*, 2002).

Current strategies to avoid the clinical side-effects of fixed orthodontic treatment are professional tooth cleaning, the local application of fluorides, and the use of antimicrobial mouth rinses (Alves *et al.*, 2008; Shafi, 2008; Tufekci *et al.*, 2008). Furthermore, sealants are used to reduce enamel decalcification (Buren *et al.*, 2008). All these strategies are focused on reducing or removing oral biofilm and are aimed at increasing the resistance of hard tissues against bacterial metabolic waste products, i.e. bacterial acids.

Despite increased preventive efforts, fixed orthodontic treatment still entails the risk of enamel demineralization (Attin *et al.*, 2005; Lovrov *et al.*, 2007). Furthermore, none of the preventive strategies have the potential to inhibit bacterial adhesion on bracket surfaces *ab initio*. Consequently, a preferable method to inhibit the detrimental effects of fixed orthodontic therapy is the development and clinical implementation of bracket surfaces with anti-adhesive characteristics.

Therefore, the objective of the present study was to compare biofilm formation on uncoated brackets with those coated with polytetrafluoroethylene (PTFE).

Subjects and methods

The present study was approved by the Ethics Committee of Hannover Medical School (No. 4347). The examination

was performed with the understanding and written consent of each participant and his/her parents.

Using nQuery Advisor 5.0 (Statistical Solutions, Saugus, Massachusetts, USA), power and sample sizes were calculated. Power calculation revealed that a sample size of four would have a power of 80 per cent to detect a difference in means of 18.2 [e.g. a first condition mean (μ_1) of 22.2 and a second condition mean (μ_2) of 4.0], assuming that the standard deviation of the differences was 7.8. In the case of the bracket debonding, the subject was considered as a dropout.

A total of 13 consecutive adolescent patients (five females and eight males, aged between 8 and 16 years, mean 11.2 ± 2.8 years) who received orthodontic treatment were included in the present study. Criteria for inclusion were need for orthodontic treatment in the late mixed dentition with symmetric primary teeth in at least one jaw. Criteria for exclusion were systemic diseases, pharmacological, or antibiotic therapy 6 weeks before the start of and/or during the study, a history of periodontal disease, excluding gingivitis, the presence of carious lesions, and congenitally missing permanent teeth. The patients were instructed not to seek professional tooth cleaning during the study and not to use antibacterial mouth rinses.

Of a total of 26 sterile brackets (Victory Series; 3M Unitek, Monrovia, California, USA), 13 were coated with food-safe PTFE after sandblasting with $54 \mu\text{m Al}_2\text{O}_3$ (Adelhelm Kunststoffbeschichtungen GmbH, Eningen, Germany). To avoid bracket debonding, PTFE was removed from the mesh by sandblasting with $110 \mu\text{m Al}_2\text{O}_3$. During this procedure, a dental silicone embedding material (Silagum; DMG Chemisch Pharmazeutische Fabrik GmbH, Hamburg, Germany) was used to protect the PTFE-coated facial surfaces. For all 26 brackets, a 0.016×0.022 inch stainless steel segment of archwire (OrthoForm; 3M Unitek) was fixed with of two elastomeric ligatures (Alastik; 3M Unitek).

In all patients, one PTFE-coated bracket and one uncoated bracket were temporarily and symmetrically bonded (Transbond; 3M Unitek) to the first or second primary molars (four maxillary and nine mandibular) for a period of 8 weeks (Figure 1a and b). Selection of the right and left quadrants was randomized using a random list. Before bracket bonding, the teeth were sandblasted for 3–4 seconds with $50 \mu\text{m Al}_2\text{O}_3$ (Microetcher; Danville Engineering, San Ramon, California, USA) and etched with orthophosphoric acid for 30 seconds (Conditioner 36; DeTrey, Konstanz, Germany).

After 8 weeks, the brackets were debonded with orthodontic pliers and the archwire, including the elastomeric ligatures, was removed. The brackets were then gently rinsed with sterile water and air-dried.

Analysis of quantitative biofilm formation was performed with the Rutherford backscattering detection (RBSD) method, a scanning electron microscopy (SEM) technique (Leo 1455 VP; Carl Zeiss SMT AG, Oberkochen, Germany). For each bracket, a total of five RBSD photomicrographs were obtained with identical views from the mesial, distal, occlusal, cervical, and buccal aspects. After obtaining the

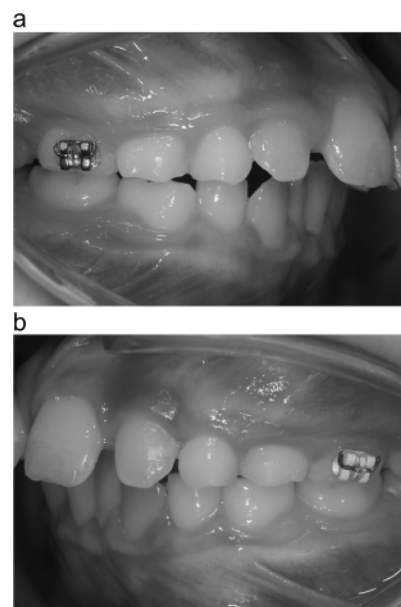


Figure 1 Intraoral view of the uncoated (a) and polytetrafluoroethylene-coated (b) premolar bracket bonded to primary second molars, including a segmented 0.016×0.022 inch stainless steel archwire and two elastic modules per bracket.

RBSD micrographs, positive findings of biofilm coverage were validated using SEM at high magnification.

The extent of biofilm-covered surfaces on the RBSD photomicrographs was calculated using surface analysis software (Image J 10.2 for Apple; National Institutes of Health, Bethesda, Maryland, USA). On these photomicrographs, biofilm coverage appears as dark areas and uncoated surfaces as bright areas as a result of different atomic weights (Figure 2a and b). Firstly, the regions of interest on each photomicrograph were marked. The threshold value for ideal representation of biofilm-covered surface in the region of interest was then determined. Depending on these different grey values, biofilm coverage was calculated for each photomicrograph after conversion to a binary display (Figure 3a–d; Chin *et al.*, 2006).

Documentation and evaluation of the data were performed with the Statistical Package for Social Sciences Version 16.0 for Windows (SPSS Inc., Chicago, Illinois, USA). Reproducibility of surface analysis was assessed by repeated measurements of 10 randomly selected photomicrographs applying the method of Bland and Altman (1986). Firstly, the means and standard deviations of absolute and relative biofilm coverage were calculated for each view of a bracket. Furthermore, total biofilm formation was calculated for both surface modifications. Data were compared using a two-sided paired *t*-test. For multiple tests, Bonferroni corrected levels of *P*-values were calculated. All tests were performed at a significance level of $\alpha = 0.05$.

Results

A total of four dropouts were recorded during the study, due to bracket loss. Therefore, analysis of quantitative biofilm

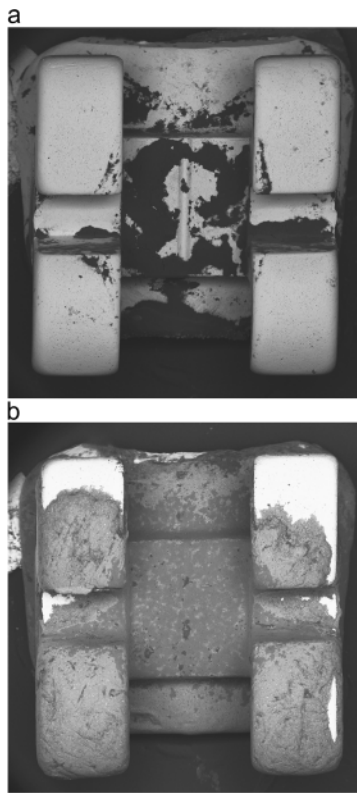


Figure 2 Rutherford backscattering detection method photomicrographs of an uncoated (a) and a polytetrafluoroethylene-coated bracket (b) as viewed from the buccal aspect. Both brackets were obtained from the same patient. Dark areas indicate adherent biofilm. The bright surfaces in Figure 2b represent abraded surfaces due to high shear forces.

formation was based on a total of 90 photomicrographs. A total area of $21.7 \pm 0.7 \text{ mm}^2$ per bracket was investigated. The results of total biofilm analysis on brackets are shown in Figure 4. On PTFE-coated brackets, total biofilm formation was 4.0 ± 3.6 per cent ($0.9 \pm 0.8 \text{ mm}^2$) of the bracket surface and on uncoated brackets 22.2 ± 5.4 per cent ($4.8 \pm 1.2 \text{ mm}^2$). The results of pairwise comparison with respect to location are shown in Table 1. For all locations, significantly less biofilm formation was found on PTFE-coated surfaces compared with stainless steel surfaces. After Bonferroni correction, the difference in biofilm formation was not significant for the cervical surfaces.

For PTFE-coated brackets, the highest values of biofilm formation were found on the mesial surfaces (6.8 ± 4.4 per cent) and the lowest on the occlusal surfaces (1.2 ± 1.2 per cent). On uncoated brackets, the greatest biofilm accumulation was present on the distal surfaces (29.7 ± 17.0 per cent), whereas the lowest values were found on the occlusal surfaces (16.0 ± 7.2 per cent).

A total of 13.9 ± 5.2 per cent ($3.0 \pm 1.2 \text{ mm}^2$) of PTFE-coated brackets were abraded. Abrasion was found in regions with high shear forces (occlusal bracket wings).

As regards the reproducibility of surface analysis, the empirical standard deviation for biofilm coverage was 0.5 ± 1.2 per cent, indicating good reproducibility.

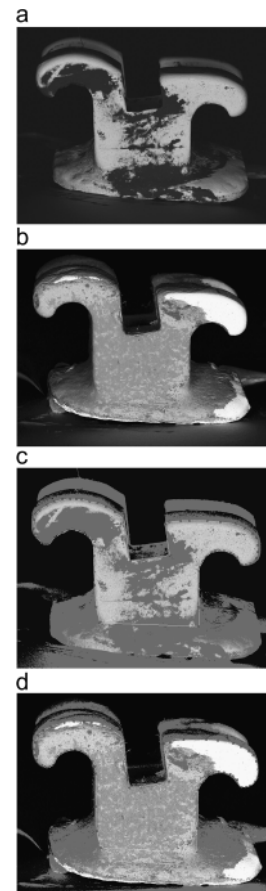


Figure 3 Converted Rutherford backscattering detection method photomicrographs of an uncoated (a) and a polytetrafluoroethylene-coated (b) bracket viewed from the approximal aspect. Biofilm coverage was calculated based on grey levels (c and d).

Discussion

In the present study, mid-term analysis of biofilm formation on orthodontic brackets was performed in adolescent patients. This age cohort was selected because it is the major treatment group in orthodontics, and these patients possess primary teeth, which can be used for study purposes without inducing lesions on permanent teeth. Primary teeth were selected for bonding, as cleaning and finishing of bonded tooth surfaces induces enamel loss of about $50 \mu\text{m}$ (Al Shamsi *et al.*, 2007). Furthermore, mechanical bracket debonding entails the risk of enamel fractures (Stratmann *et al.*, 1996). As clinical studies involving adolescents are associated with ethical concerns, sample size was reduced to the minimum with respect to statistical requirements.

Biofilm formation on alloplastic materials endangers the integration of medical devices and the integrity of human tissues. Consequently, the clinical implementation of anti-adhesive and antibacterial surfaces for medical purposes are a major goal in current research (Fu *et al.*, 2006; Coughlan *et al.*, 2008). PTFE was selected as the coating in the present study since clinical research has shown that the use of PTFE coatings reduces bacterial adhesion on medical devices (Berry *et al.*,

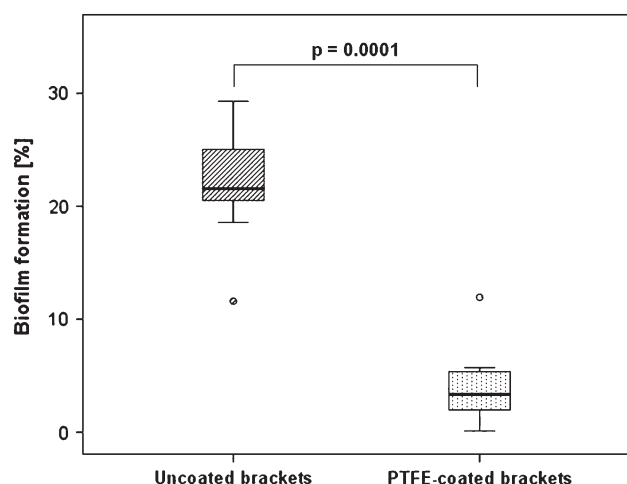


Figure 4 Total biofilm formation of uncoated and polytetrafluoroethylene-coated brackets.

Table 1 Mean values and comparison of biofilm formation on uncoated and polytetrafluoroethylene (PTFE)-coated surfaces with respect to location (per cent).

	Uncoated	PTFE coated	P-value	P-value (Bonferroni)
Buccal	17.7±4.4	2.7±3.2	0.0001	0.0005
Occlusal	16.0±7.2	1.2±1.2	0.0001	0.0005
Cervical	21.8±11.7	6.4±9.5	0.043	0.215
Mesial	28.1±9.9	6.8±4.4	0.0001	0.0005
Distal	29.7±17.0	3.8±3.1	0.001	0.005

2000). So far, PTFE has been used in the field of orthodontics to reduce the frictional resistance between the archwire and the bracket slot, but not as an anti-adhesive coating to reduce biofilm formation (De Franco *et al.*, 1995; Husmann *et al.*, 2002; Bortoly *et al.*, 2008). The PTFE was white coloured to demonstrate that an anti-adhesive coating also fulfils aesthetic demands of patients during fixed orthodontic treatment.

An archwire segment was engaged using elastic ligatures in all brackets to provide an environment with plaque-retentive sites that can be compared with treatment conditions. Elastic ligatures are known to induce an increase in biofilm accumulation (Turkkahraman *et al.*, 2005). Iatrogenic biofilm dislodgement during the removal process was reduced by minimizing the contact surface when placing the pliers on the bracket wings. To ensure biofilm formation that can be compared with long-term orthodontic treatment, the investigation was performed over the specific period of 8 weeks (Ristic *et al.*, 2007).

In the present study, quantitative analysis of biofilm formation on brackets was performed using the RBSD technique and surface analysis software. This method has been previously used to detect biofilm on supra- and subgingival surfaces of orthodontic bands and dental implant abutments (Elter *et al.*, 2008; Demling *et al.*, 2009). With the RBSD technique, element-contrast photomicrographs are obtained by

showing surfaces with low atomic weight (such as oral biofilms) as darker grey values than surfaces with higher atomic weight (such as stainless steel). The representation of three-dimensional structures such as brackets in two-dimensional photographs results in distortion. In this study, the problem of distortion was overcome, as the photomicrographs were obtained from identical views, data were compared pairwise, and relative biofilm formation was compared.

On uncoated brackets, biofilm was found on 22.2 ± 5.4 per cent of the surfaces. This amount of biofilm is comparable with that on other intraoral alloplastic materials, such as titanium (Heuer *et al.*, 2007). On uncoated brackets, the biofilm was mostly located on surfaces that are not accessible with a toothbrush or the tongue. These findings can be explained by reduced shear forces in these regions, where bacteria are protected from mechanical removal and hydrodynamic effects such as saliva flow or movement of oral soft tissues (Quirynen and Bollen, 1995; Hannig, 1999).

In contrast, only 4.0 ± 3.6 per cent of the coated surfaces were covered with biofilm. Even on occult and covered surfaces, hardly any biofilm was found on coated brackets. These results can be explained by the material characteristics of PTFE, which consists of carbon and fluorine, and can be chemically described as a fluoropolymer. These fluorocarbons exhibit a high electronegativity and, as a consequence, are not susceptible to dispersive factors, such as Van der Waals forces. The exploitation of dispersive forces is considered to be the predominant attachment mechanism for microorganisms on hard intraoral surfaces (Eliades *et al.*, 1995).

Results of biofilm analysis showed a relatively high standard deviation, representing interindividual differences in the amount of biofilm-covered surfaces. This can be explained by covariables, such as nutrition, tongue activity, and oral hygiene.

Pairwise comparison of data showed a significantly lower biofilm formation for all bracket locations. These results demonstrate that the anti-adhesive effect of a biofilm-reducing PTFE coating can be found on the complete bracket. However, after Bonferroni correction, the differences were not significant for the cervical surfaces. The values for biofilm formation on cervical surfaces indicate that in a larger cohort, significant differences between uncoated and PTFE-coated brackets would also have been found for this location.

On surfaces with high shear forces, the PTFE coating was partially abraded. The coated brackets used in this research must be considered prototypes. Long-term stability of the PTFE coating might be improved by application of other coating techniques or selective coating of surfaces with low shear forces (Luo *et al.*, 2008).

Conclusions

Uncoated orthodontic brackets are highly susceptible to biofilm formation that endangers the integrity of oral hard and soft tissues by means of decalcification and periodontal disease. A PTFE coating on brackets reduced the biofilm

formation to a minimum. Although the coating was partially abraded on surfaces exposed to high shear forces, the results of the study are encouraging. In the future, coatings with long-term stability could contribute to reduced biofilm accumulation on fixed orthodontic appliances.

Address for correspondence

Dr Anton Demling
Department of Orthodontics
Hannover Medical School
Carl-Neuberg-Strasse 1
30625 Hannover
Germany
E-mail: demling.anton@mh-hannover.de

References

- Ahn S J, Lim B S, Lee S J 2007 Prevalence of cariogenic streptococci on incisor brackets detected by polymerase chain reaction. *American Journal of Orthodontics and Dentofacial Orthopedics* 131: 736–741
- Al Shamsi A H, Cunningham J L, Lamey P J, Lynch E 2007 Three-dimensional measurement of residual adhesive and enamel loss on teeth after debonding of orthodontic brackets: an *in-vitro* study. *American Journal of Orthodontics and Dentofacial Orthopedics* 131: e309–e315
- Alves P V, Alviano W S, Bolognese A M, Nojima L I 2008 Treatment protocol to control *Streptococcus mutans* level in an orthodontic patient with high caries risk. *American Journal of Orthodontics and Dentofacial Orthopedics* 133: 91–94
- Anhoury P, Nathanson D, Hughes C V, Socransky S, Feres M, Chou L L 2002 Microbial profile on metallic and ceramic bracket materials. *Angle Orthodontist* 72: 338–343
- Atack N E, Sandy J R, Addy M 1996 Periodontal and microbiological changes associated with the placement of orthodontic appliances. A review. *Journal of Periodontology* 67: 78–85
- Attin R *et al.* 2005 Recolonization of *mutans streptococci* on teeth with orthodontic appliances after antimicrobial therapy. *European Journal of Orthodontics* 27: 489–493
- Berry J A, Biedlingmaier J F, Whelan P J 2000 *In vitro* resistance to bacterial biofilm formation on coated fluoroplastic tympanostomy tubes. *Otolaryngology Head and Neck Surgery* 123: 246–251
- Bland J M, Altman D G 1986 Statistical methods for assessing agreement between two methods of clinical measurement. *The Lancet* 1: 307–310
- Bortoly T G, Guerrero A P, Rached R N, Tanaka O, Guariza-Filho O, Rosa E A 2008 Sliding resistance with esthetic ligatures: an *in-vitro* study. *American Journal of Orthodontics and Dentofacial Orthopedics* 133: 340.e1–e7
- Boyd R L 1983 Longitudinal evaluation of a system for self-monitoring plaque control effectiveness in orthodontic patients. *Journal of Clinical Periodontology* 10: 380–388
- Buren J L, Staley R N, Wefel J, Qian F 2008 Inhibition of enamel demineralization by an enamel sealant, Pro Seal: an *in-vitro* study. *American Journal of Orthodontics and Dentofacial Orthopedics* 133: 88–94
- Chin M Y, Busscher H J, Evans R, Noar J, Pratten J 2006 Early biofilm formation and the effects of antimicrobial agents on orthodontic bonding materials in a parallel plate flow chamber. *European Journal of Orthodontics* 28: 1–7
- Coughlan A, Boyd D, Douglas C W, Towler M R 2008 Antibacterial coatings for medical devices based on glass polyalkenoate cement chemistry. *Journal of Materials Science: Materials in Medicine* 19: 3555–3560
- De Franco D J, Spiller R E Jr., von Fraunhofer J A 1995 Frictional resistances using Teflon-coated ligatures with various bracket-archwire combinations. *Angle Orthodontist* 65: 63–72
- Demling A *et al.* 2009 Analysis of supra- and subgingival long-term biofilm formation on orthodontic bands. *European Journal of Orthodontics* 31: 202–206
- Eliades T, Eliades G, Brantley W A 1995 Microbial attachment on orthodontic appliances: I. Wettability and early pellicle formation on bracket materials. *American Journal of Orthodontics and Dentofacial Orthopedics* 108: 351–360
- Elter C *et al.* 2008 Supra- and subgingival biofilm formation on implant abutments with different surface characteristics. *International Journal of Oral and Maxillofacial Implants* 23: 327–334
- Fournier A, Payant L, Bouclin R 1998 Adherence of *Streptococcus mutans* to orthodontic brackets. *American Journal of Orthodontics and Dentofacial Orthopedics* 114: 414–417
- Fu J, Ji J, Fan D, Shen J 2006 Construction of antibacterial multilayer films containing nanosilver via layer-by-layer assembly of heparin and chitosan-silver ions complex. *Journal of Biomedical Materials Research A* 79: 665–674
- Hannig M 1999 Transmission electron microscopy of early plaque formation on dental materials *in vivo*. *European Journal of Oral Sciences* 107: 55–64
- Heuer W *et al.* 2007 Analysis of early biofilm formation on oral implants in man. *Journal of Oral Rehabilitation* 34: 377–382
- Husmann P, Bourauel C, Wessinger M, Jäger A 2002 The frictional behavior of coated guiding archwires. *Journal of Orofacial Orthopedics* 63: 199–211
- Lovrov S, Hertrich K, Hirschfelder U 2007 Enamel demineralization during fixed orthodontic treatment—incidence and correlation to various oral-hygiene parameters. *Journal of Orofacial Orthopedics* 68: 353–363
- Luo Z *et al.* 2008 Stable bionic superhydrophobic coating surface fabricated by a conventional curing process. *Advanced Materials* 20: 970–974
- Naranjo A A, Trivino M L, Jaramillo A, Betancourth M, Botero J E 2006 Changes in the subgingival microbiota and periodontal parameters before and 3 months after bracket placement. *American Journal of Orthodontics and Dentofacial Orthopedics* 130: 275.e17–e22
- Øgaard B 1989 Prevalence of white spot lesions in 19-year-olds: a study on untreated and orthodontically treated persons 5 years after treatment. *American Journal of Orthodontics and Dentofacial Orthopedics* 96: 423–427
- Quirynen M, Bollen C M 1995 The influence of surface roughness and surface-free energy on supra- and subgingival plaque formation in man. A review of the literature. *Journal of Clinical Periodontology* 22: 1–14
- Ristic M, Vlahovic Svabic M,asic M, Zelic O 2007 Clinical and microbiological effects of fixed orthodontic appliances on periodontal tissues in adolescents. *Orthodontics and Craniofacial Research* 10: 187–195
- Sallum E J *et al.* 2004 Clinical and microbiologic changes after removal of orthodontic appliances. *American Journal of Orthodontics and Dentofacial Orthopedics* 126: 363–366
- Shafi I 2008 Fluoride varnish reduces white spot lesions during orthodontic treatment. *Evidence-Based Dentistry* 9: 81
- Stratmann U, Schaarschmidt K, Wegener H, Ehmer U 1996 The extent of enamel surface fractures. A quantitative comparison of thermally debonded ceramic and mechanically debonded metal brackets by energy dispersive micro- and image-analysis. *European Journal of Orthodontics* 18: 655–662
- Tang E L, Wei S H 1990 Assessing treatment effectiveness of removable and fixed orthodontic appliances with the occlusal index. *American Journal of Orthodontics and Dentofacial Orthopedics* 98: 550–556
- Tufekci E, Casagrande Z A, Lindauer S J, Fowler C E, Williams K T 2008 Effectiveness of an essential oil mouthrinse in improving oral health in orthodontic patients. *Angle Orthodontist* 78: 294–298
- Turkkahraman H, Sayin M O, Bozkurt F Y, Yetkin Z, Kaya S, Onal S 2005 Archwire ligation techniques, microbial colonization, and periodontal status in orthodontically treated patients. *Angle Orthodontist* 75: 231–236
- van Gastel J, Quirynen M, Teughels W, Coucke W, Carels C 2008 Longitudinal changes in microbiology and clinical periodontal variables after placement of fixed orthodontic appliances. *Journal of Periodontology* 79: 2078–2086

Copyright of European Journal of Orthodontics is the property of Oxford University Press / UK and its content may not be copied or emailed to multiple sites or posted to a listserv without the copyright holder's express written permission. However, users may print, download, or email articles for individual use.